



CHI150 Saturated Calomel Electrode (SCE)

Introduction



$E^0 = 0.241\text{V}$ vs NHE at 25°C for saturated calomel electrode (SCE)

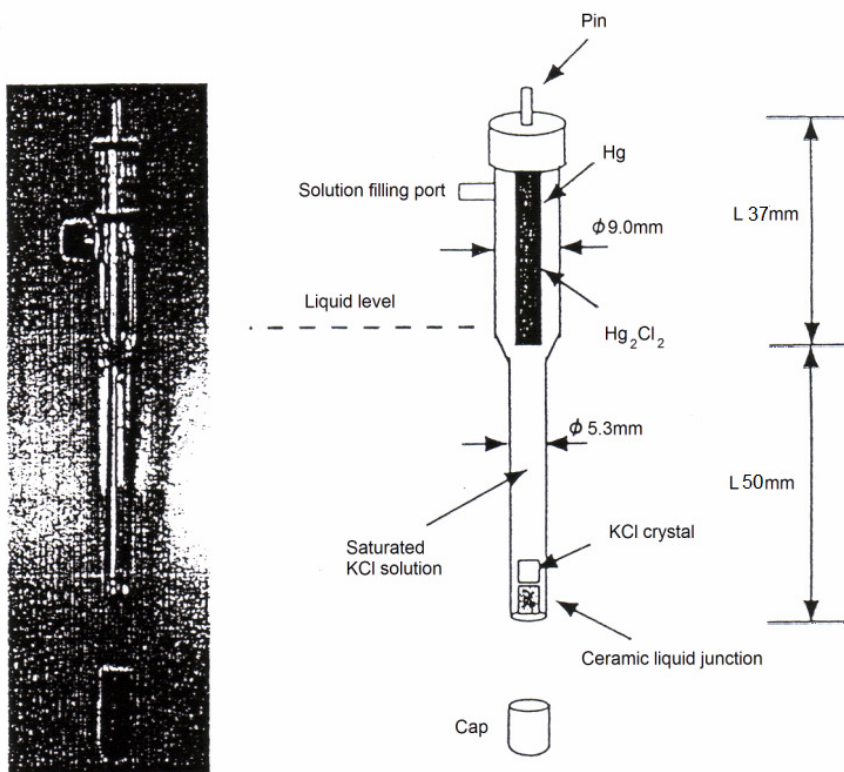

Note:

1. Please remove cap before first time use.
2. If there is air bubbles trapped in the chamber, please swing the electrode body to remove air bubbles.
3. If the solution inside the electrode is below the liquid level shown above, please fill saturated KCl solution.
4. After use, please dip the electrode into saturated KCl solution.

CH Instruments, Inc.
3700 Tennon Hill Drive
Austin, TX 78738 USA
Tel: (512) 402-0176 Fax: (512) 402-0186
E-mail: info@chinstruments.com